





1/5

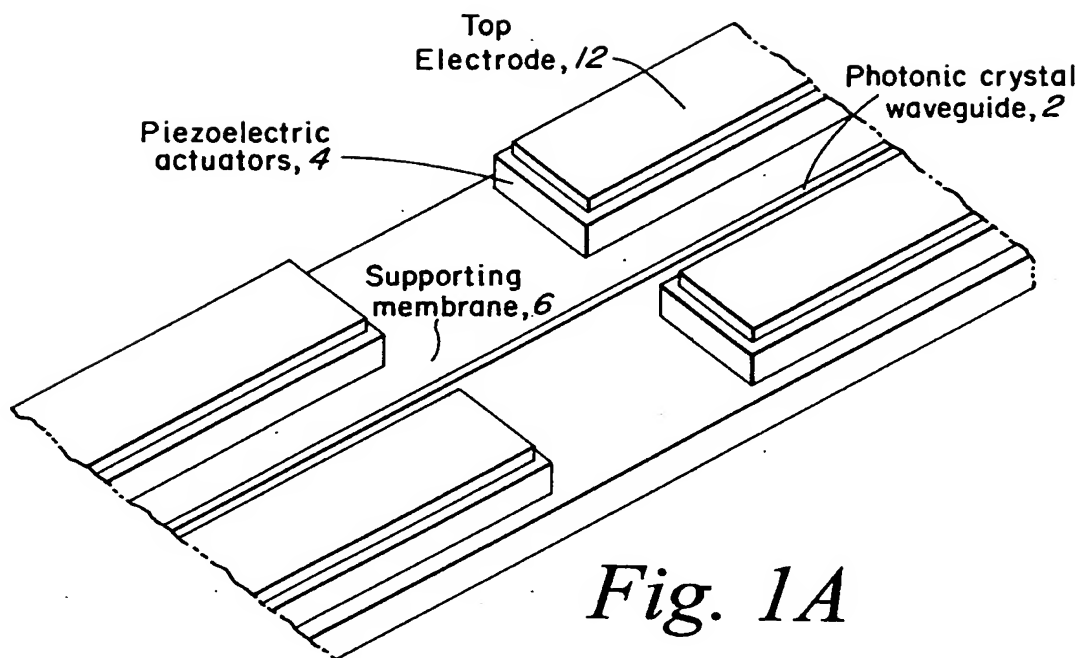


*Fig. 1A*

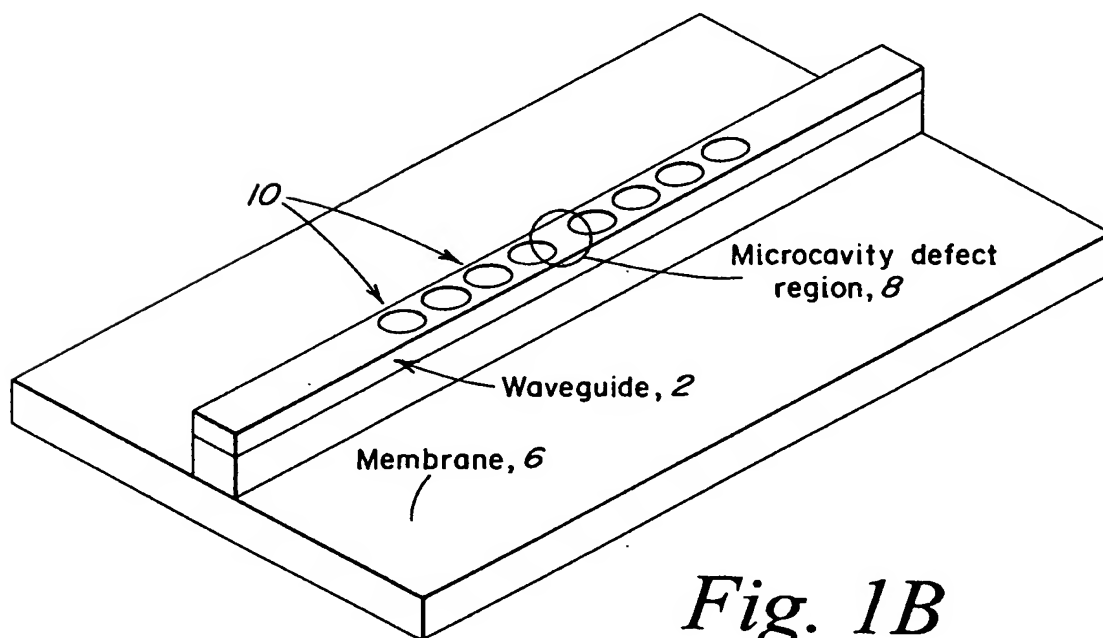

*Fig. 1B*



2/5

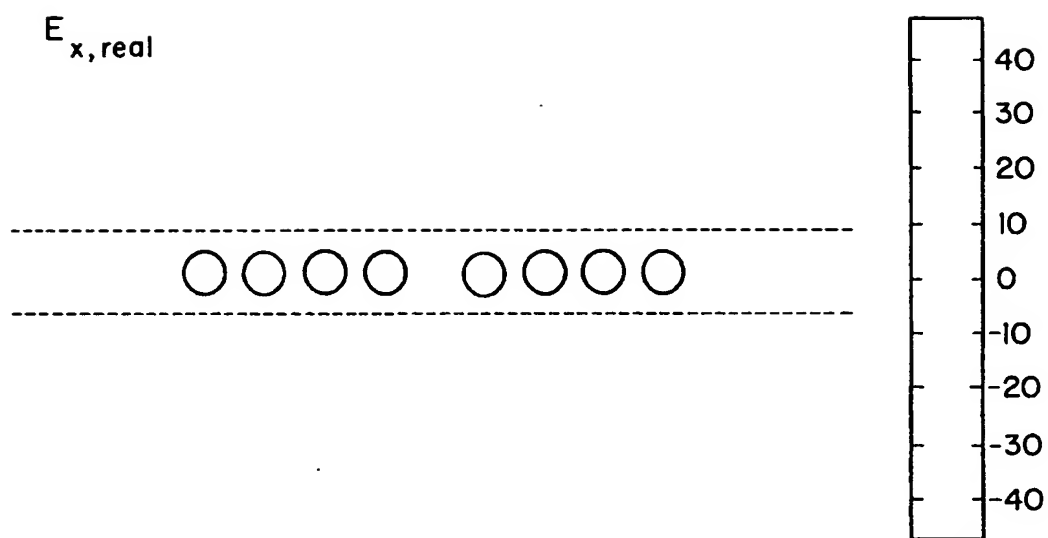

*Fig. 2*



3/5

STRAIN II  
RST CALC  
TIME 1.000

0.002100
0.001500
0.000900
0.000300
-0.000300
-0.000900
-0.001500



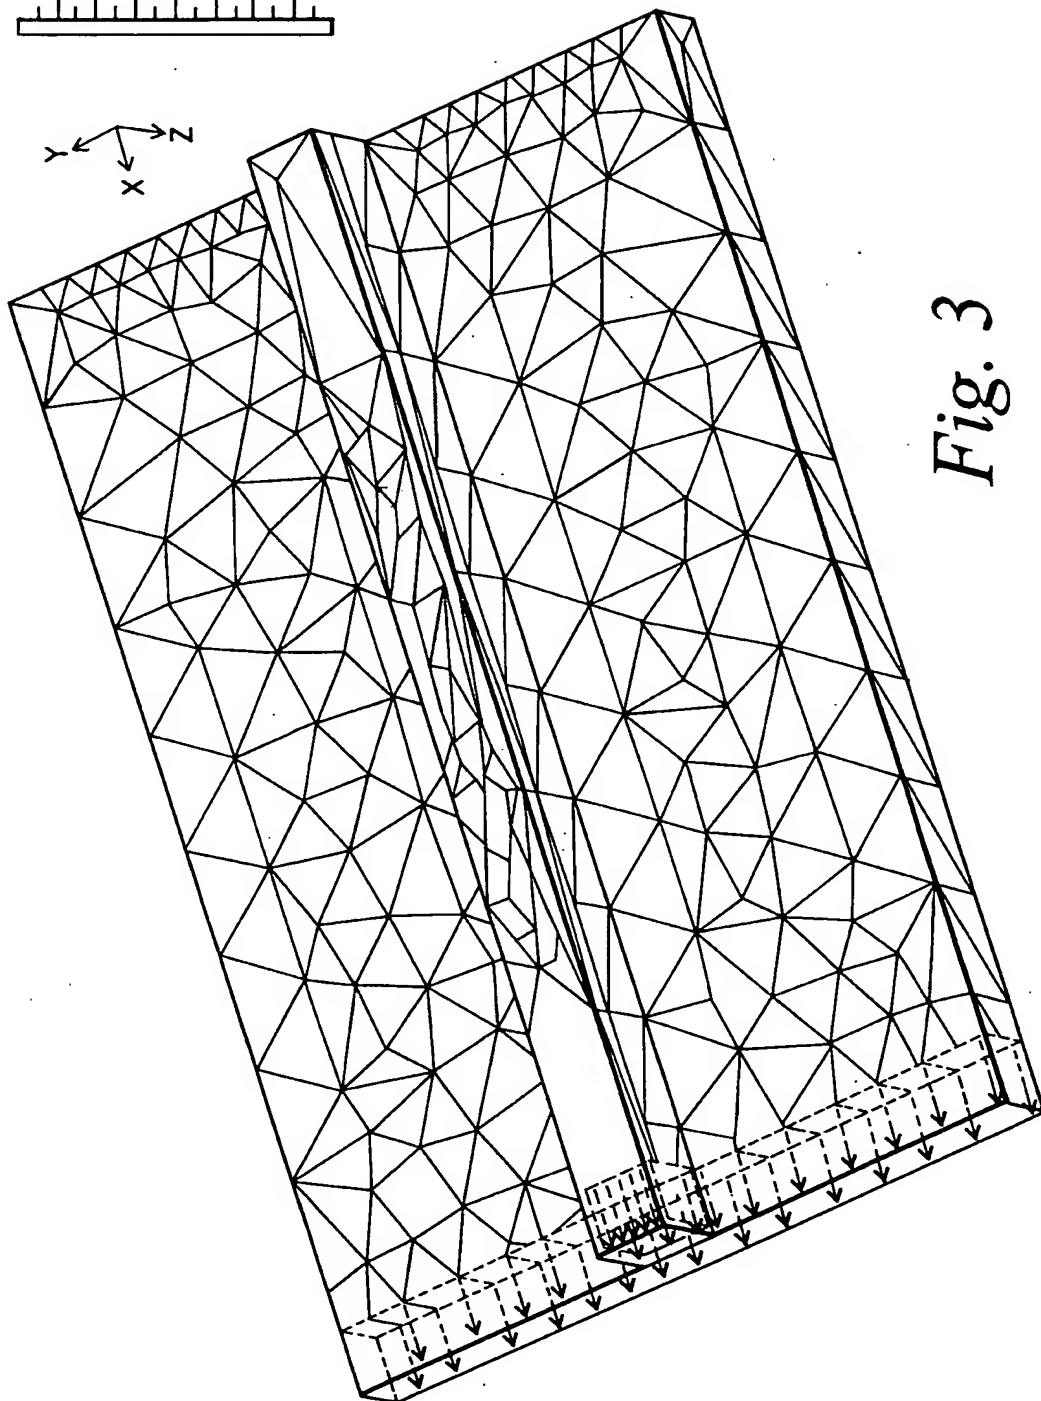


Fig. 3


4/5

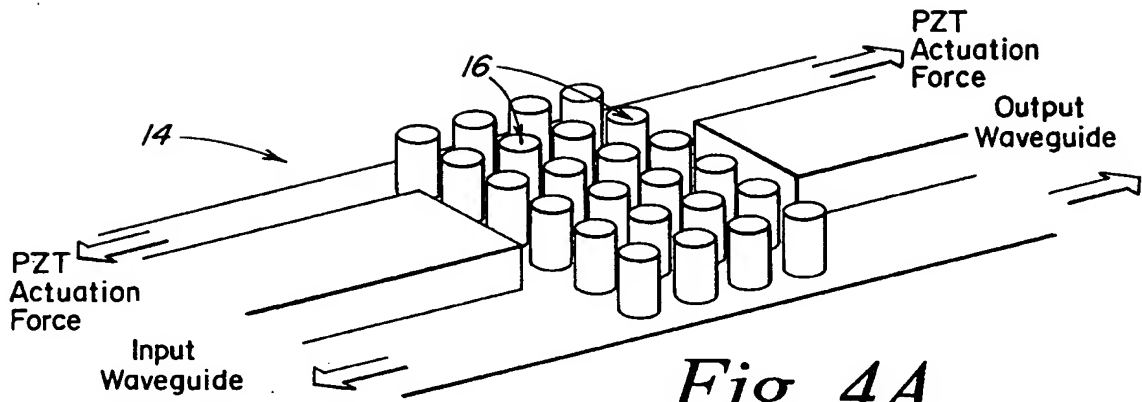

*Fig. 4A*

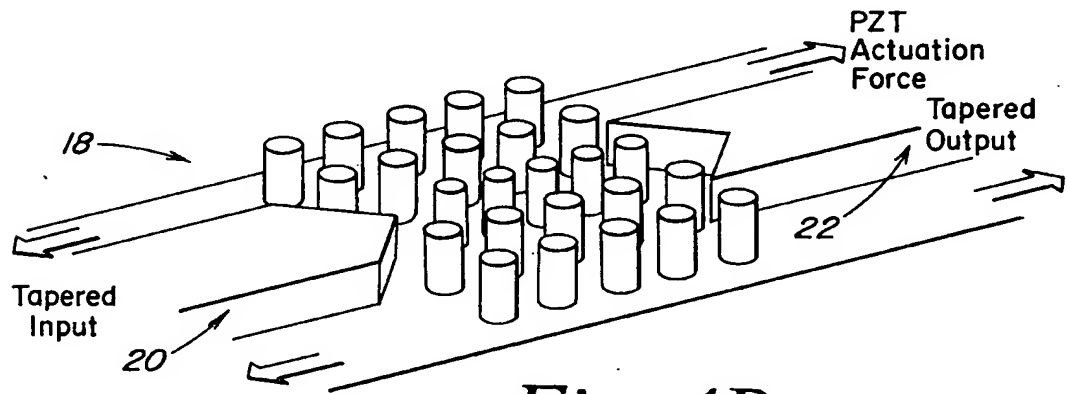


*Fig. 4B*

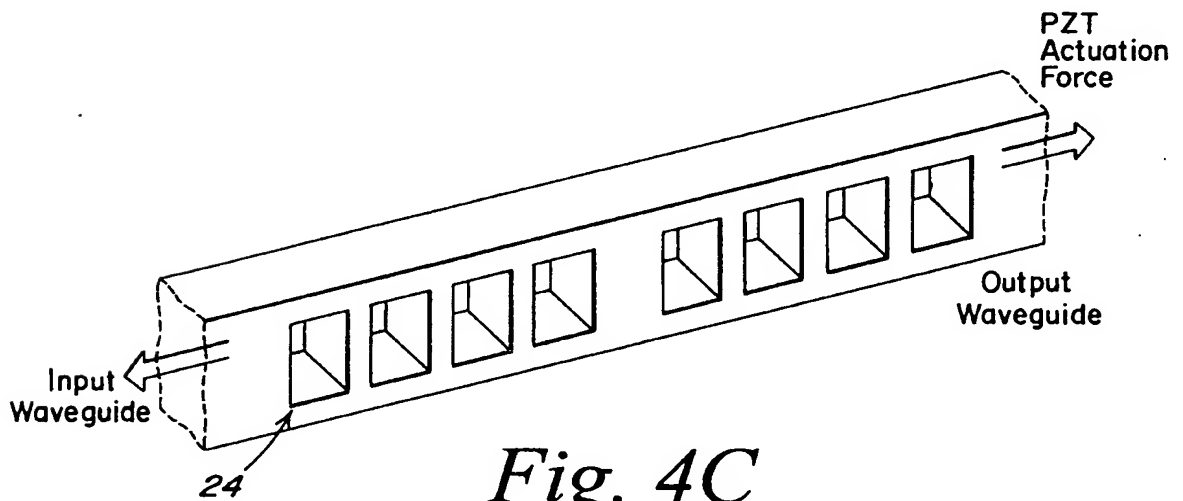

*Fig. 4C*



5/5

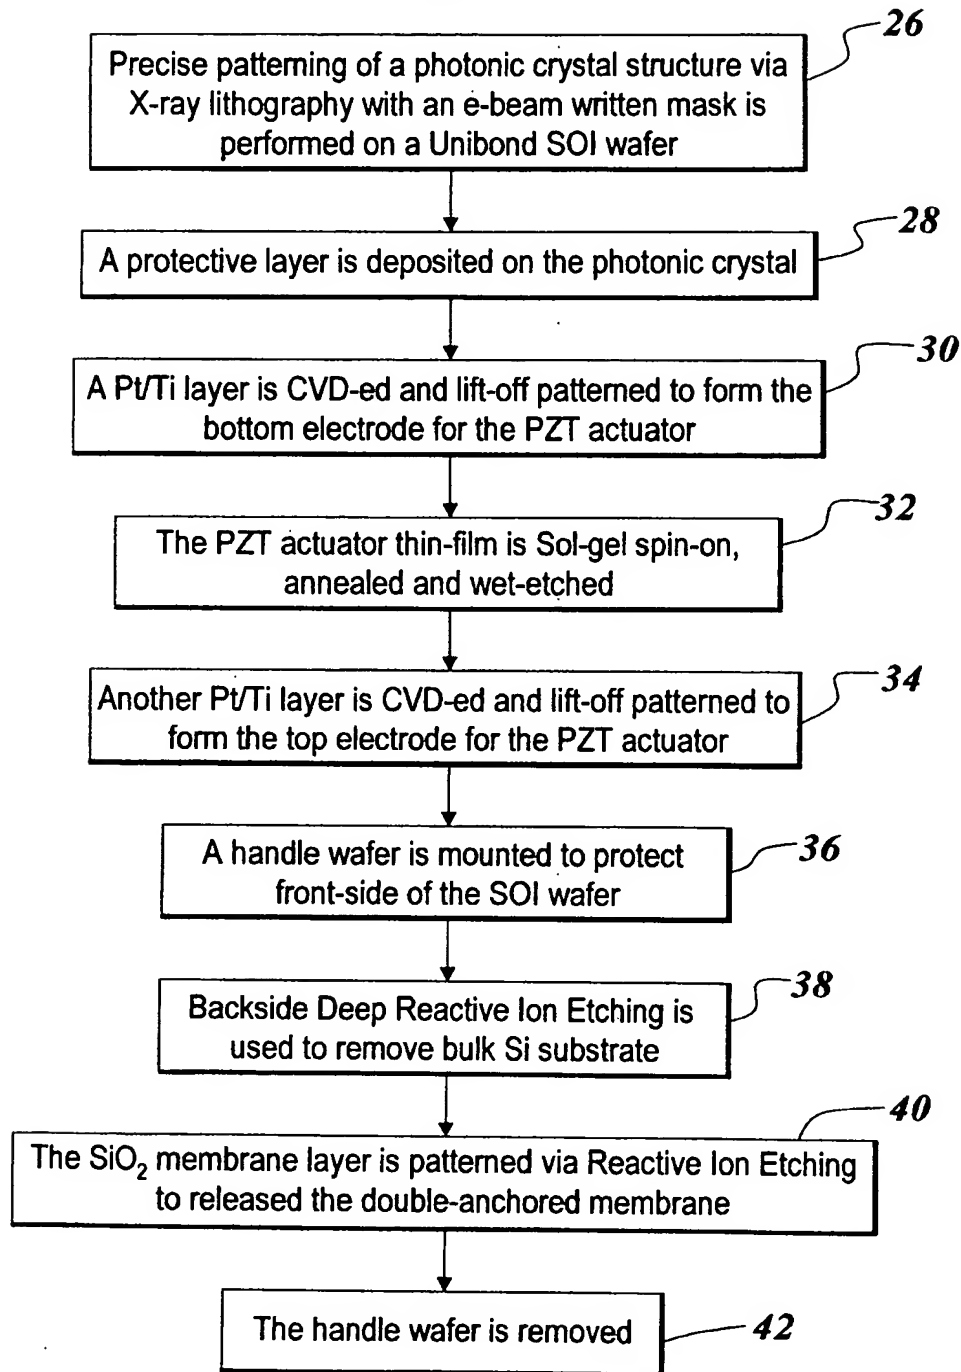

*Fig. 5*